


Third angle projection



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.




ASHCROFT INC.
250 EAST MAIN STREET,
STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019

Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]




SCALE 1:4

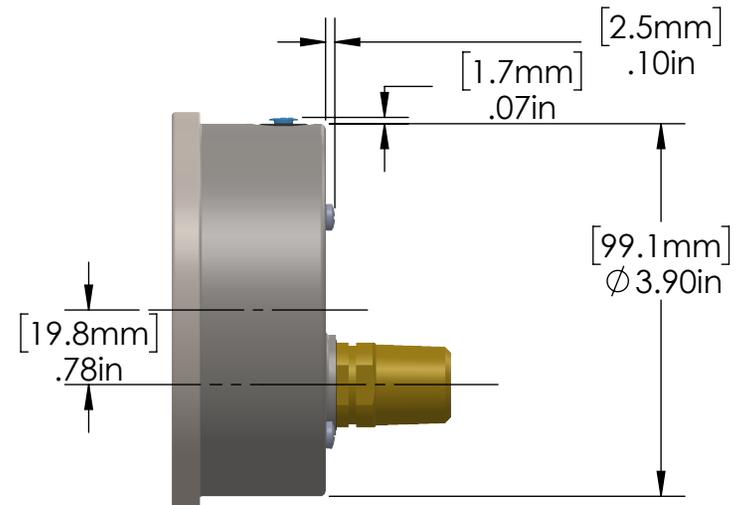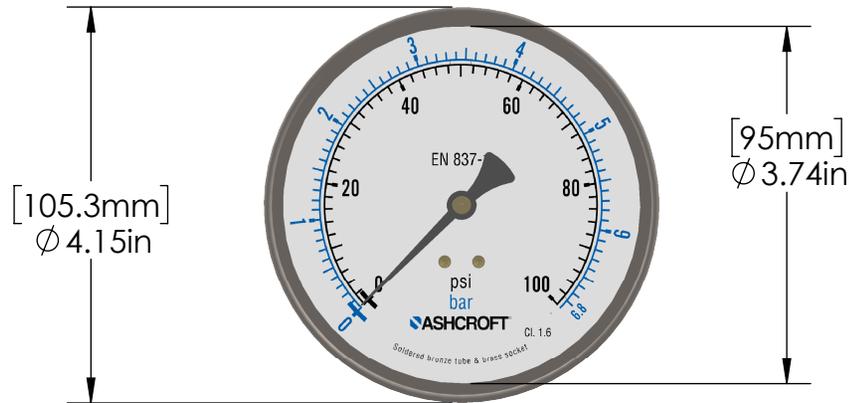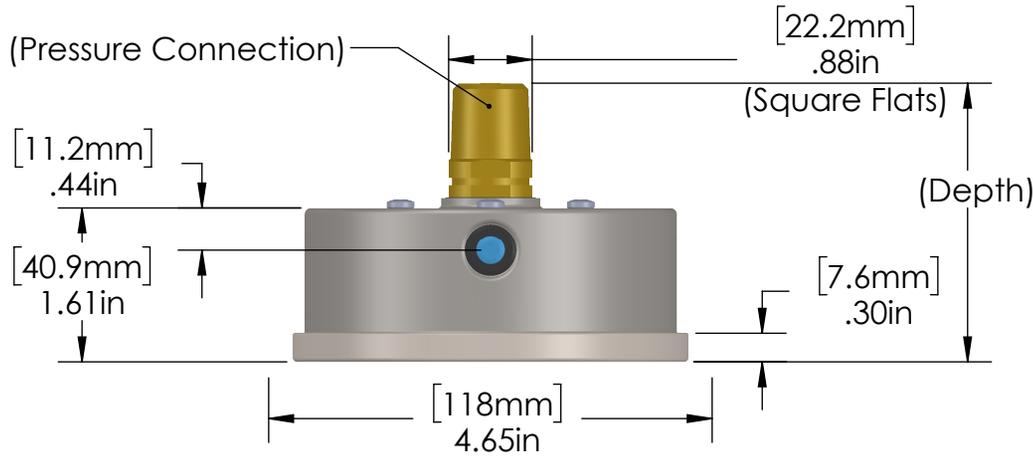

(04 Connection Shown)

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge 100mm Lower Back Connection Mounting Code "0" [Stem Mount]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-1	Rev.
Certified by	Date			070A4128	B



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT^{INC.}
 250 EAST MAIN STREET,
 STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019




Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]



SCALE 1:4


Recommended Panel Hole Size

MIN: 3.94in [100.0mm]
MAX: 4.02in [102.0mm]

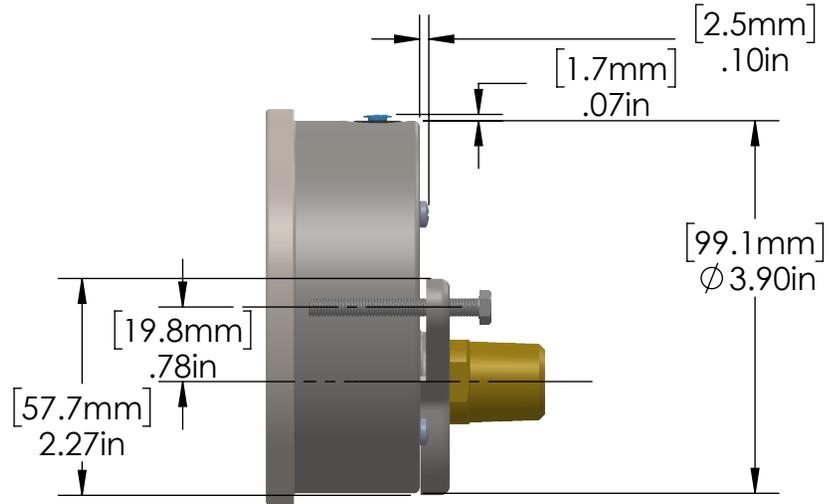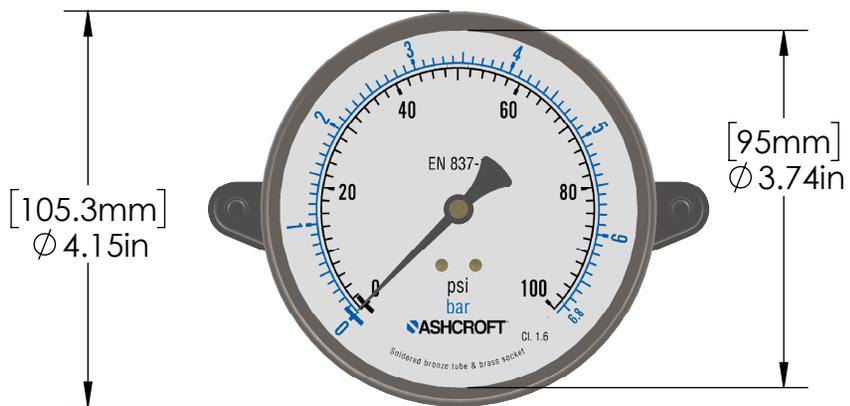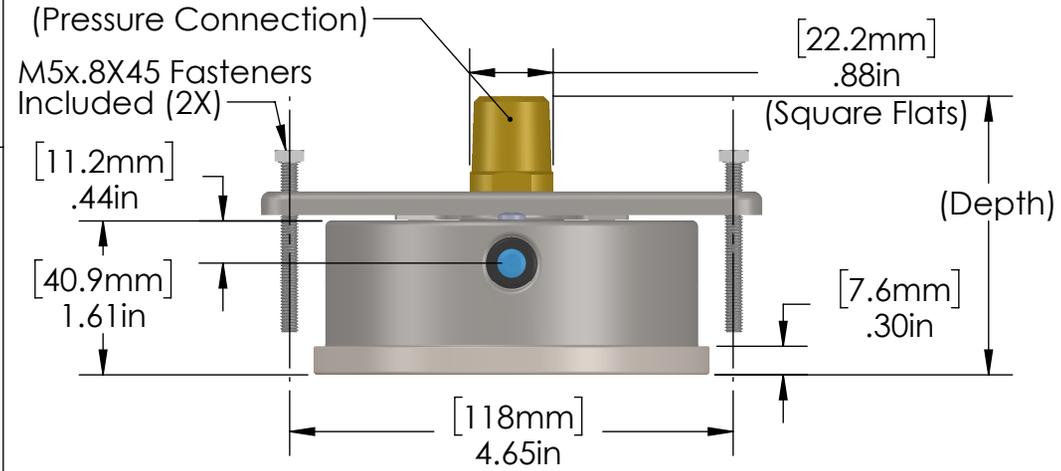

(04 Connection Shown)

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "1" [Panel Mount (Socket)]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-2	
Certified by		Date		070A4128	B



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT^{INC.}
 250 EAST MAIN STREET,
 STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019




Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]




SCALE 1:4

Recommended Panel Hole Size

MIN: 4.04in [102.5mm]
MAX: 4.15in [105.4mm]

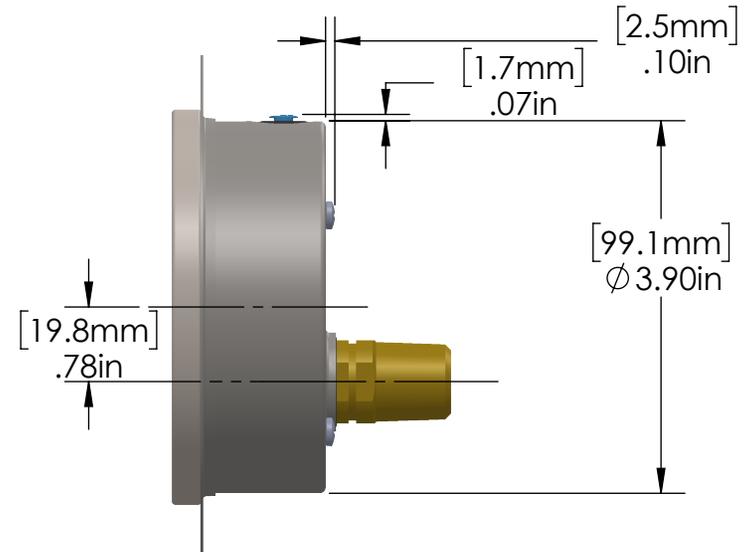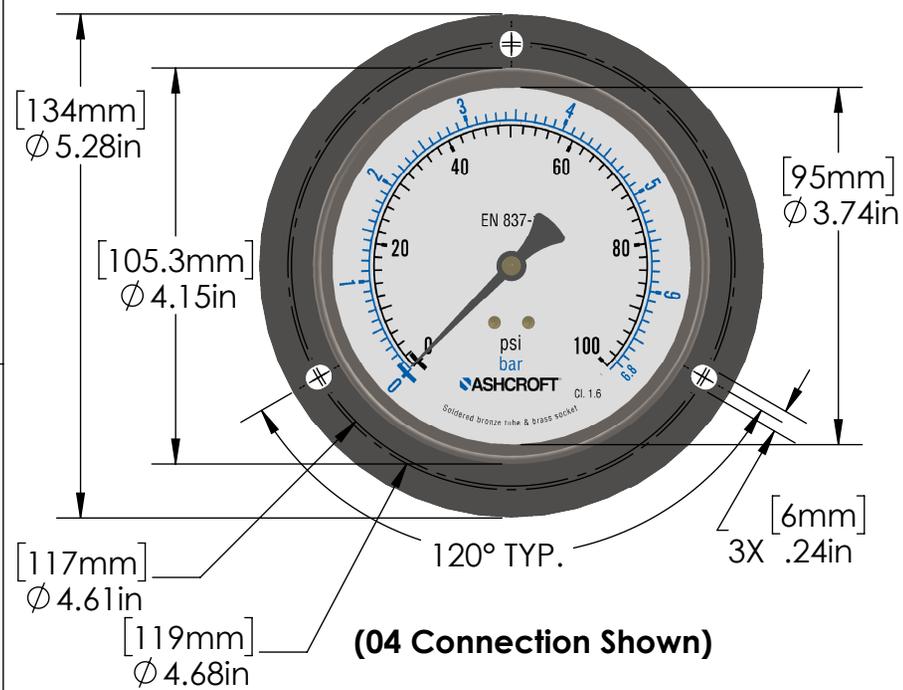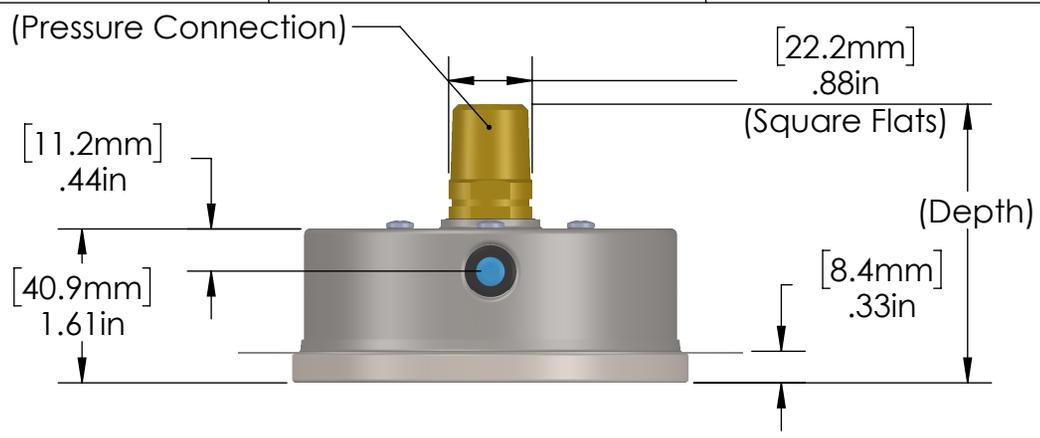

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "2" [Front Flange]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-3	
Certified by		Date		070A4128	B



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT^{INC.}
 250 EAST MAIN STREET,
 STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019




Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]



SCALE 1:4


Recommended Panel Hole Size

MIN: 4.04in [102.5mm]
MAX: 4.15in [105.4mm]

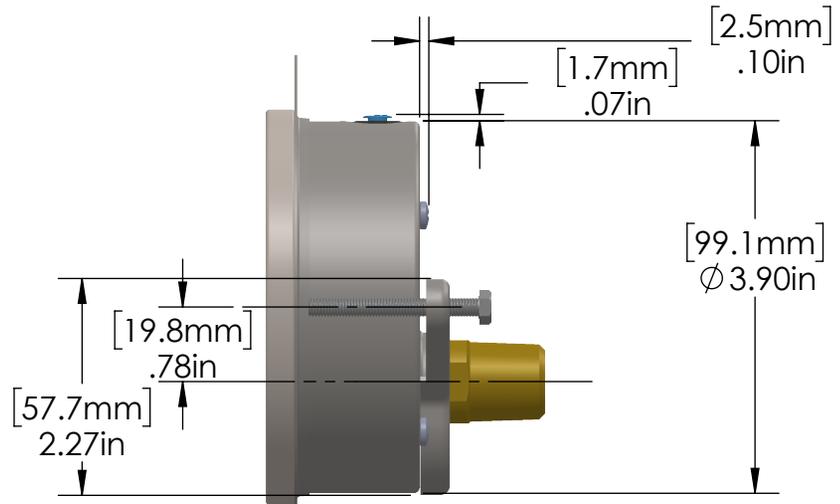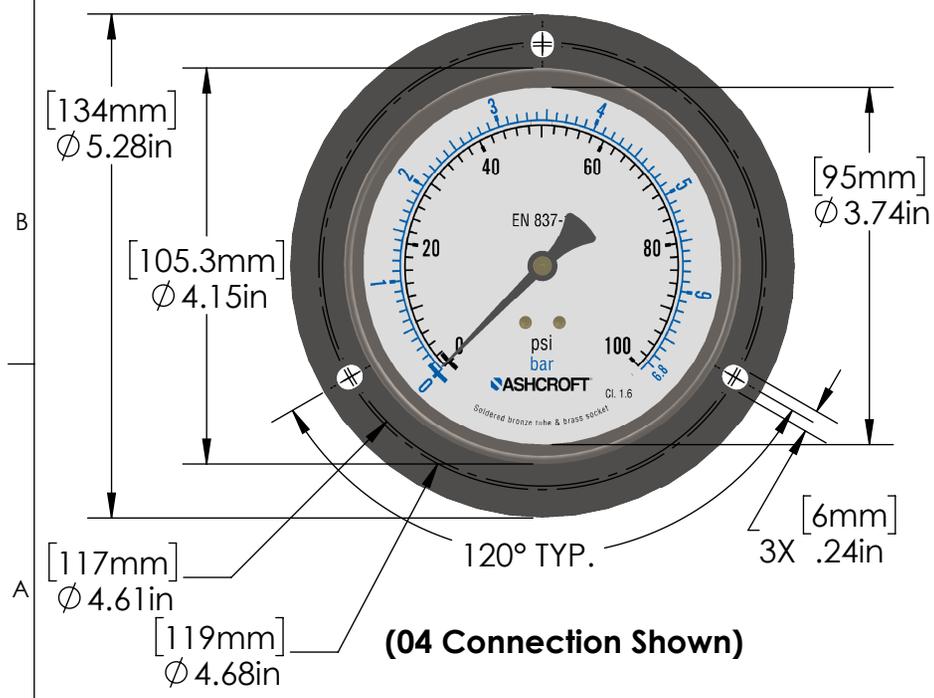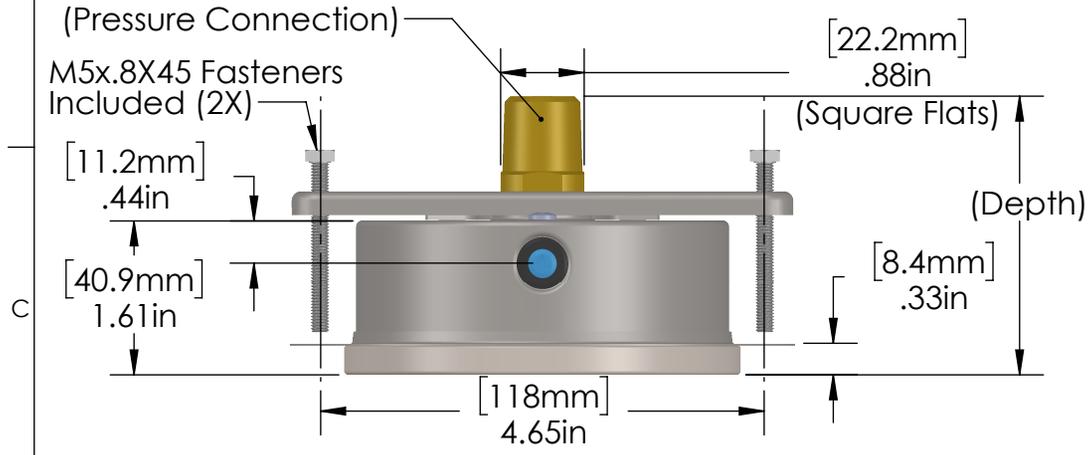

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "4" [Panel Mount (Socket) & Front Flange]			
Customer's Order No.	Drawn	Date	Date of Issue		
Ashcroft Order No.	Patel, Priyank	3/5/2019	SHEET-4		Rev.
Certified by	Date			070A4128	B

Third angle projection



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT^{INC.}
250 EAST MAIN STREET,
STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019



Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]




SCALE 1:4

Recommended Panel Hole Size


MIN: 4.04in [102.5mm]
MAX: 4.15in [105.4mm]

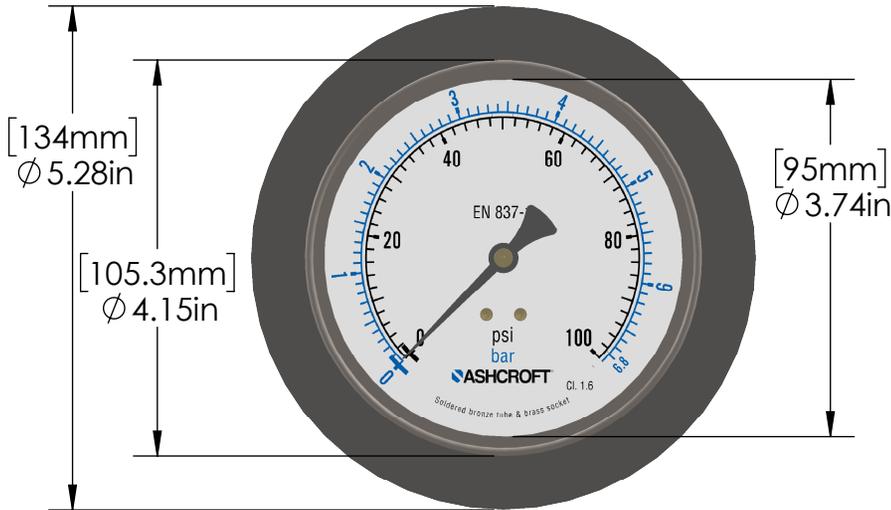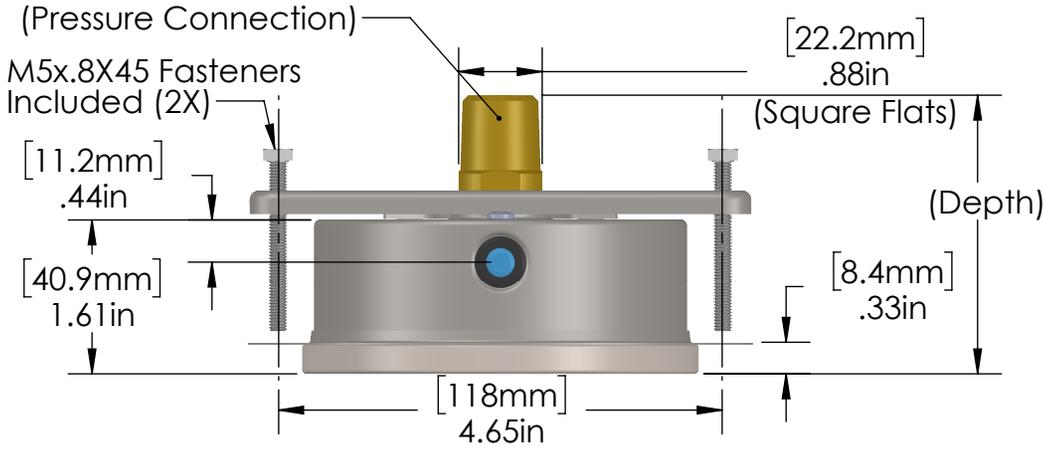

(04 Connection Shown)

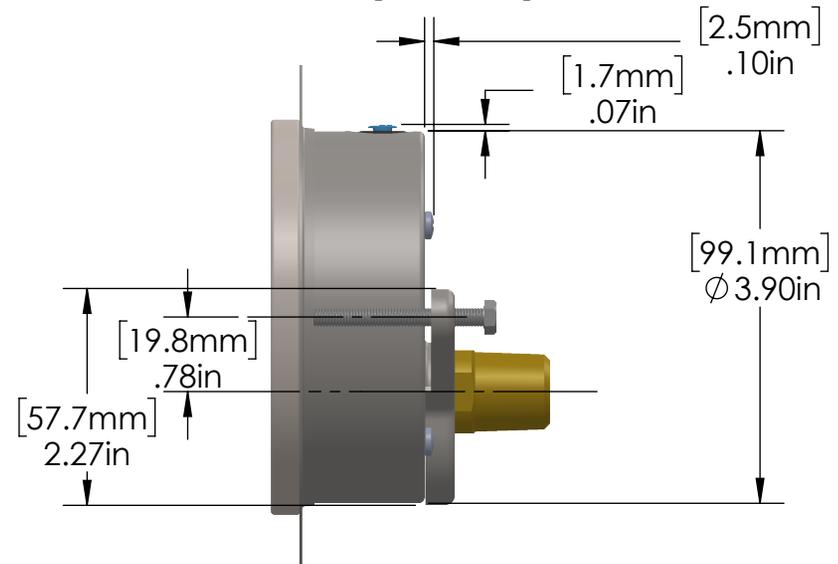

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "5" [Panel Mount (Socket) & Trim Ring]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-5	
Certified by		Date		070A4128	B



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT INC.
250 EAST MAIN STREET,
STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019




Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]



SCALE 1:4

Recommended Panel Hole Size


MIN: 3.94in [100.0mm]
MAX: 4.02in [102.0mm]

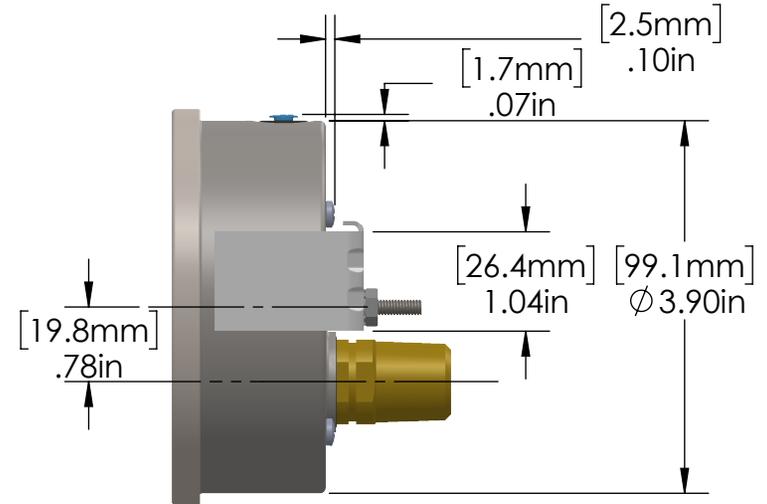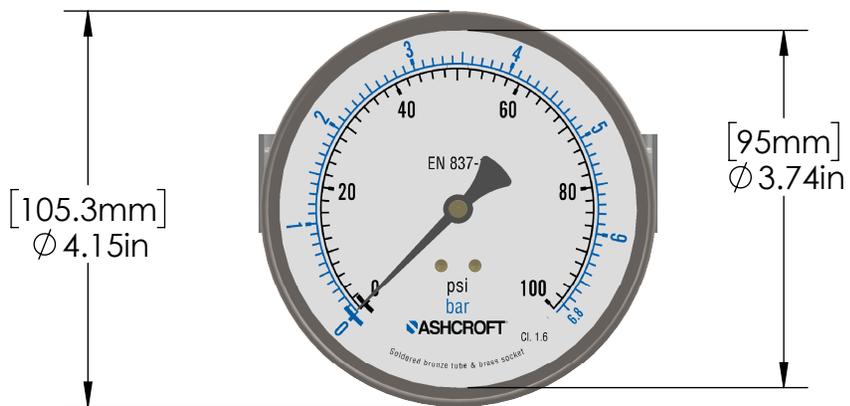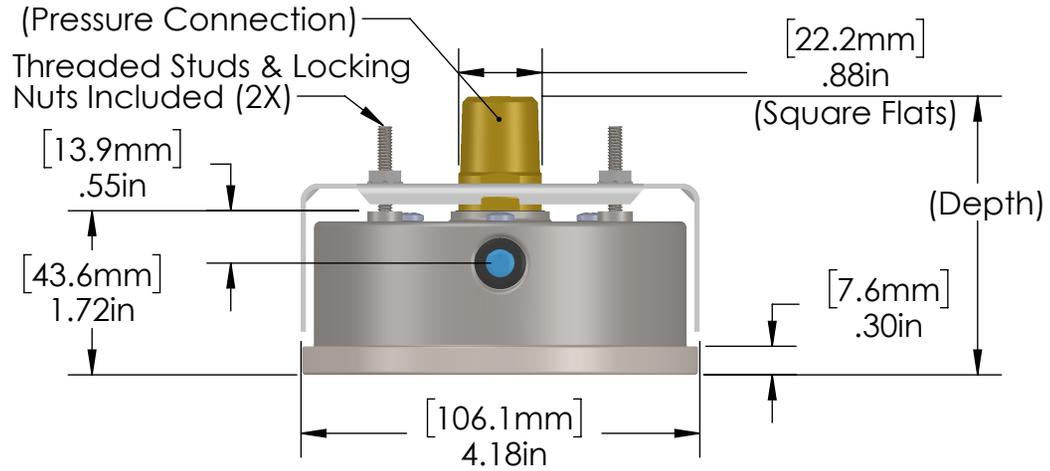

(04 Connection Shown)

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "6" [Panel Mount (Case)]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-6	
Certified by		Date		070A4128	B

Third angle projection



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT^{INC.}
250 EAST MAIN STREET,
STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019



Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]




SCALE 1:4

Recommended Panel Hole Size


MIN: 4.04in [102.5mm]
MAX: 4.15in [105.4mm]

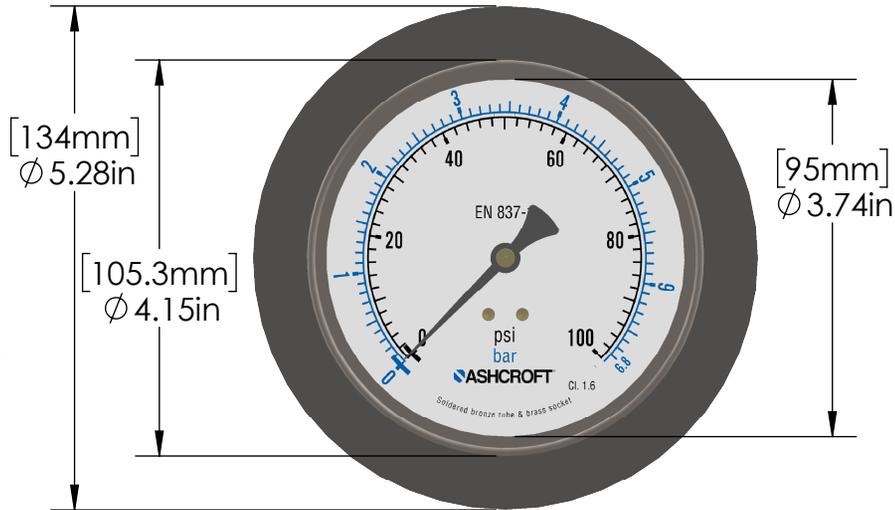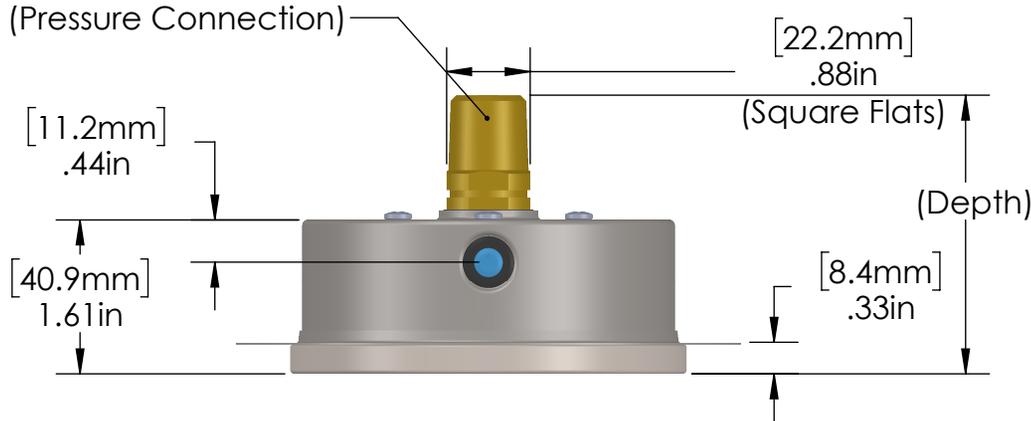

(04 Connection Shown)

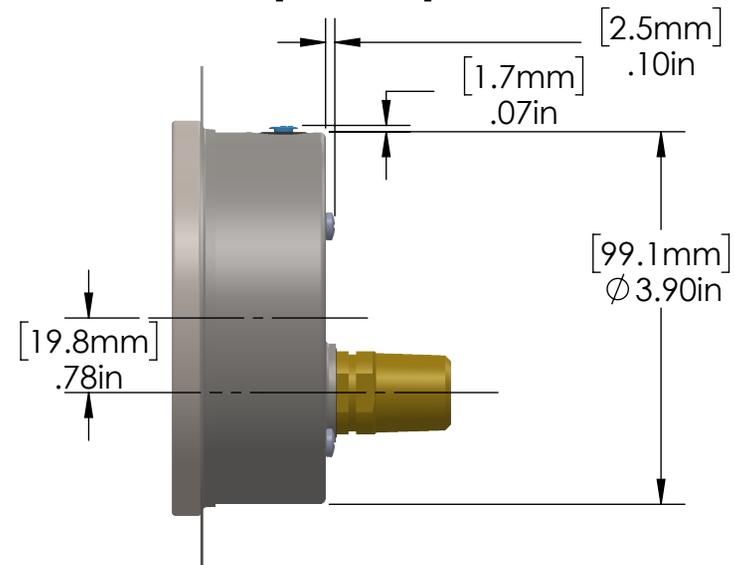

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge 100mm Lower Back Connection Mounting Code "7" [Trim Ring]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-7	Rev.
Certified by	Date			070A4128	B



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT INC.
250 EAST MAIN STREET,
STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019




Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]




SCALE 1:4

Recommended Panel Hole Size

MIN: 4.04in [102.5mm]
MAX: 4.15in [105.4mm]

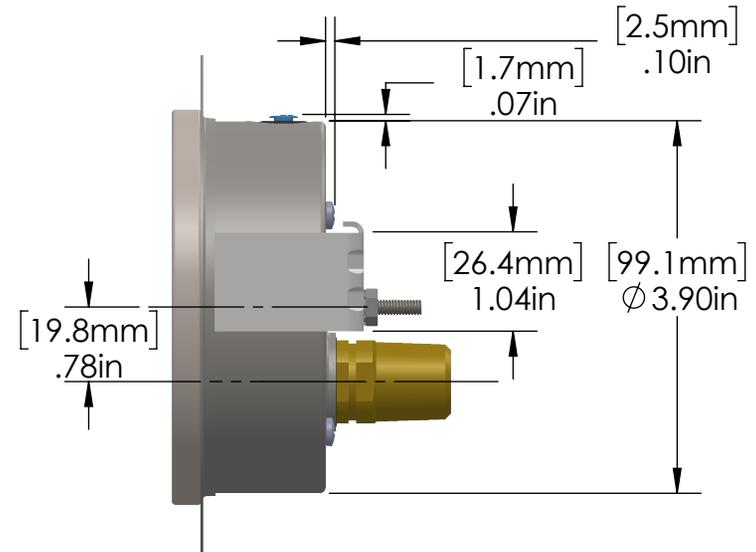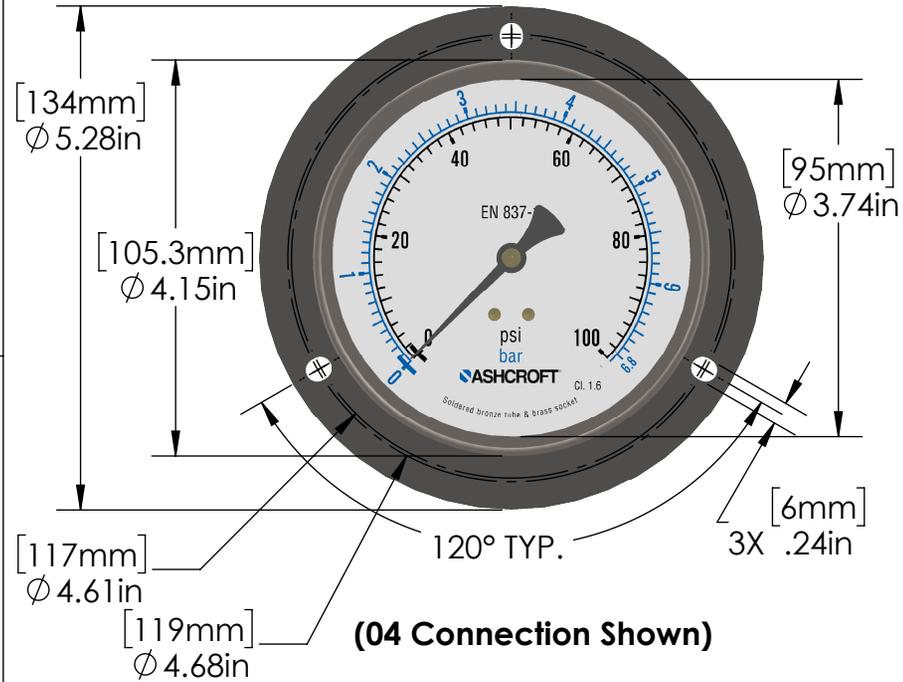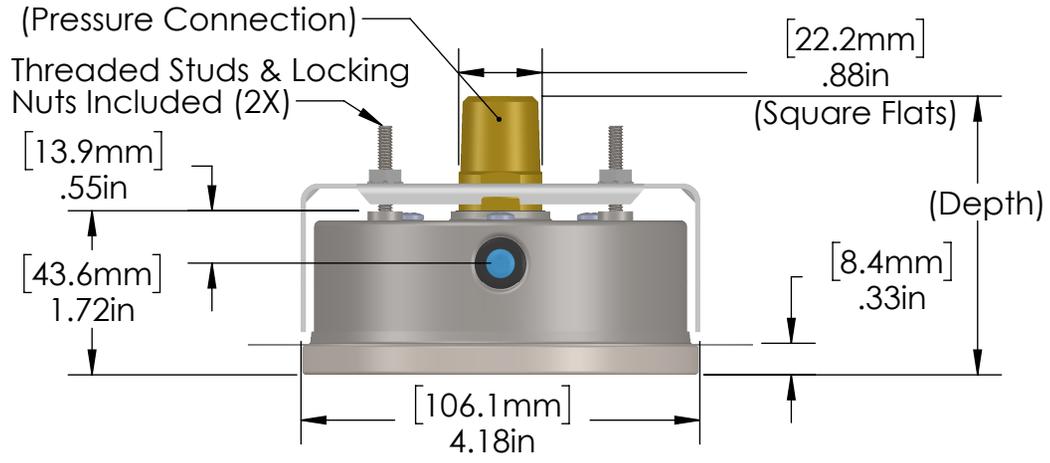

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "8" [Panel Mount (Case) & Front Flange]			
Customer's Order No.		Drawn	Date	Date of Issue	
Ashcroft Order No.		Patel, Priyank	3/5/2019	SHEET-8	
Certified by		Date		070A4128	B



This drawing includes confidential information which is the property of ASHCROFT INC. This copy is loaned for the specific purpose, with the understanding that it will not be reproduced or used for any other purpose or disclosed to others, and it will be returned on demand.

ASHCROFT INC.
250 EAST MAIN STREET,
STRATFORD, CT 06614

REV	ECO	DESCRIPTION	BY	DATE
A	8845	Initial Release	CMB	9/7/2016
B	9983	Changes to: Case OD, Ring ID	CMB	3/22/2019



Connection Code	Pressure Connection	Depth in [mm]
02	1/4 NPT	2.82 [71.6]
04	1/2 NPT	2.92 [74.1]
13	G1/4B	2.69 [68.3]
15	G1/2B	3.01 [76.3]
41	M14x1.5	2.81 [71.4]
16	M20x1.5	3.01 [76.3]
KA	1/4 BSPT	2.73 [69.3]
KD	1/2 BSPT	2.92 [74.1]




SCALE 1:4

Recommended Panel Hole Size

MIN: 4.04in [102.5mm]
MAX: 4.15in [105.4mm]

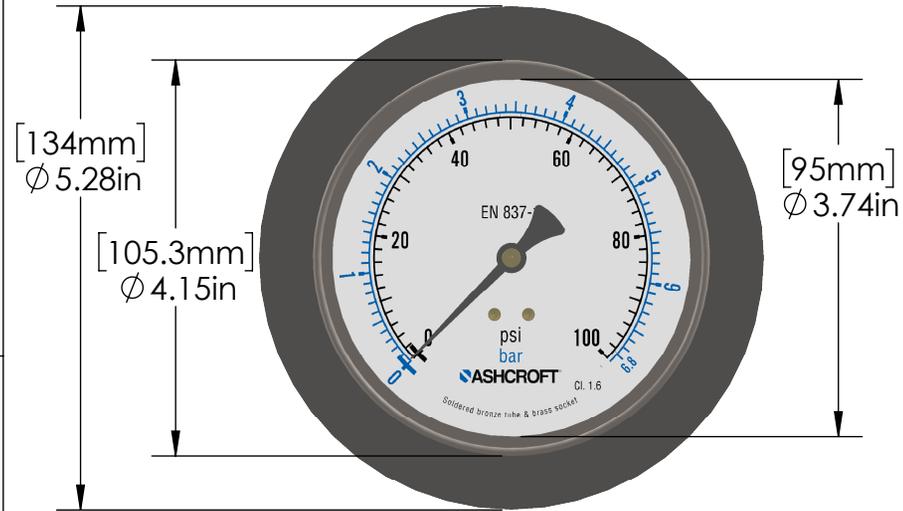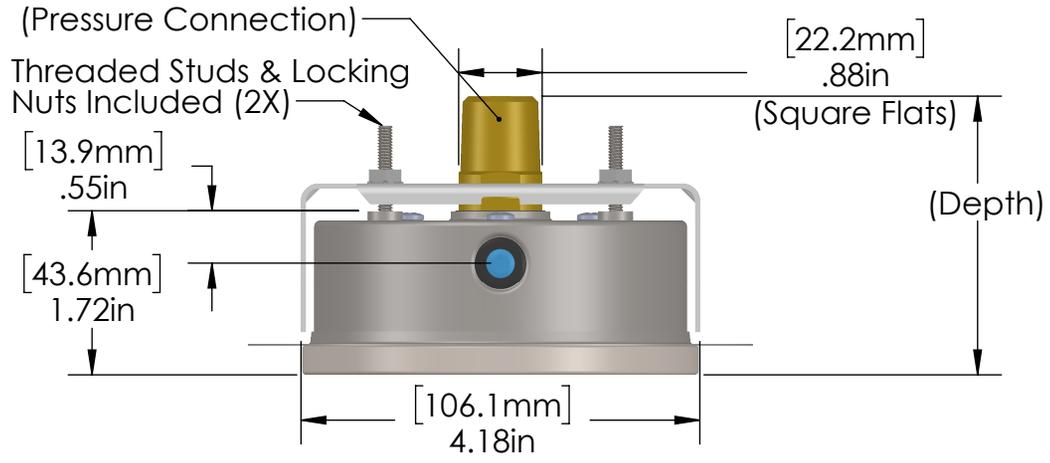

(04 Connection Shown)

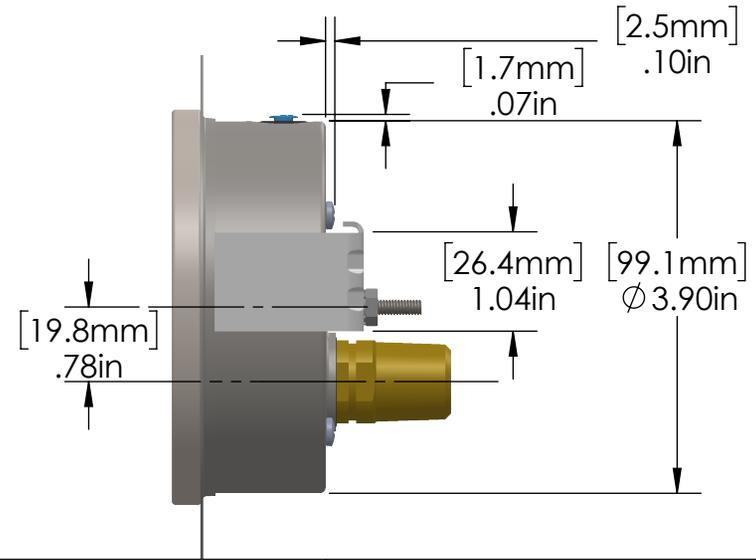

This print certified correct for		General Dimensions			
Customer's Name		8008A Series Gauge			
		100mm Lower Back Connection			
		Mounting Code "9" [Panel Mount (Case) & Trim Ring]			
Customer's Order No.	Drawn	Date	Date of Issue		
Ashcroft Order No.	Patel, Priyank	3/5/2019	SHEET-9		Rev.
Certified by	Date		070A4128		B